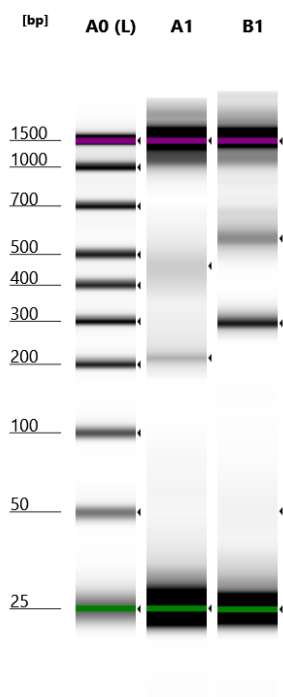



Filename: 2022-09-20-GollerMeiklejohn_CustMiSeqLibs.D1000


Default image (Contrast 50%), Image is Scaled to Sample

Sample Info

Well	Conc. [ng/ul]	Sample Description	Alert	Observations
A0	20.3	Electronic Ladder		Ladder
A1	0.426	Goller 100181390		
B1	1.16	Meiklejohn 100181016		

A0: Electronic Ladder

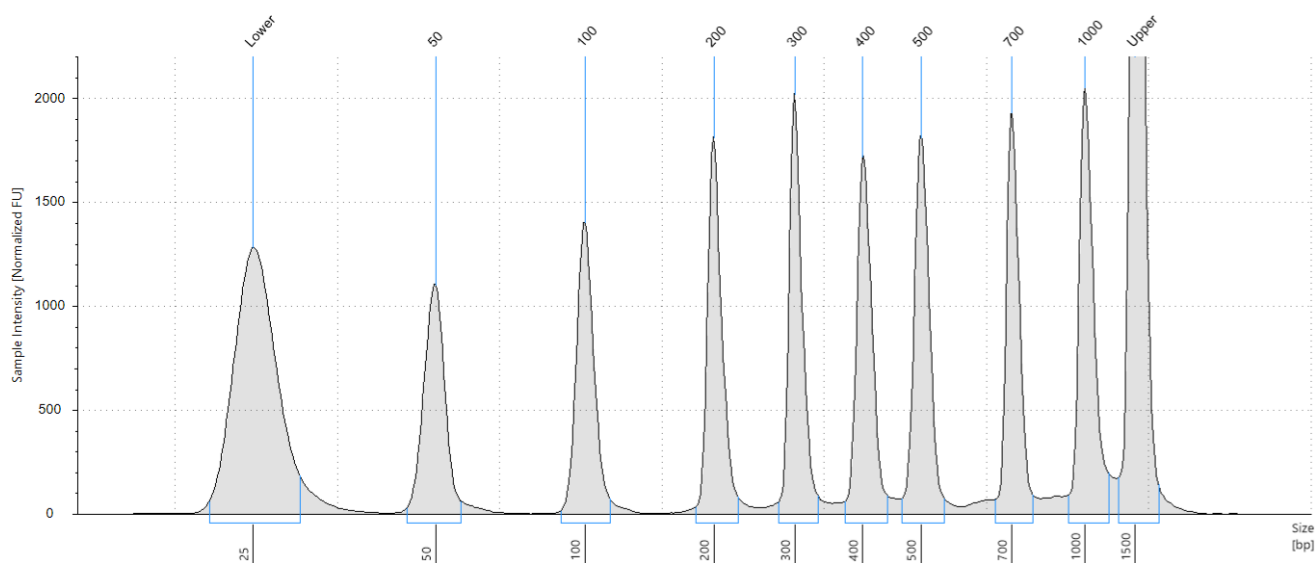


Sample Table

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
A0	20.3	Electronic Ladder		Ladder

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	5.22	-	321	-		Lower Marker
50	2.25	-	69.3	11.11		
100	2.37	-	36.5	11.71		
200	2.47	-	19.0	12.20		
300	2.55	-	13.1	12.56		
400	2.57	-	9.87	12.66		
500	2.71	-	8.33	13.36		
700	2.46	-	5.41	12.15		
1000	2.89	-	4.44	14.25		
1500	6.50	6.50	6.67	-		Upper Marker

A1: Goller 100181390

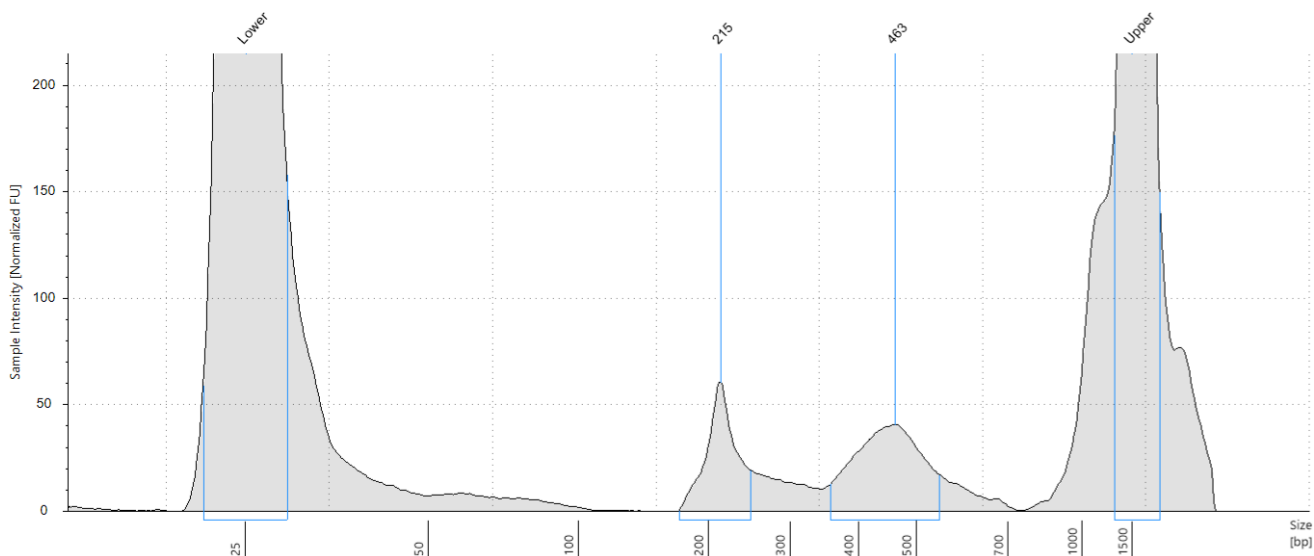


Sample Table

Well	Conc. [ng/μl]	Sample Description	Alert	Observations
A1	0.426	Goller 100181390		

Peak Table

Size [bp]	Calibrated Conc. [ng/μl]	Assigned Conc. [ng/μl]	Peak Molarity [nmol/l]	% Integrated Area	Peak Comment	Observations
25	4.32	-	266	-		Lower Marker
215	0.163	-	1.17	38.25		
463	0.263	-	0.874	61.75		
1500	6.50	6.50	6.67	-		Upper Marker

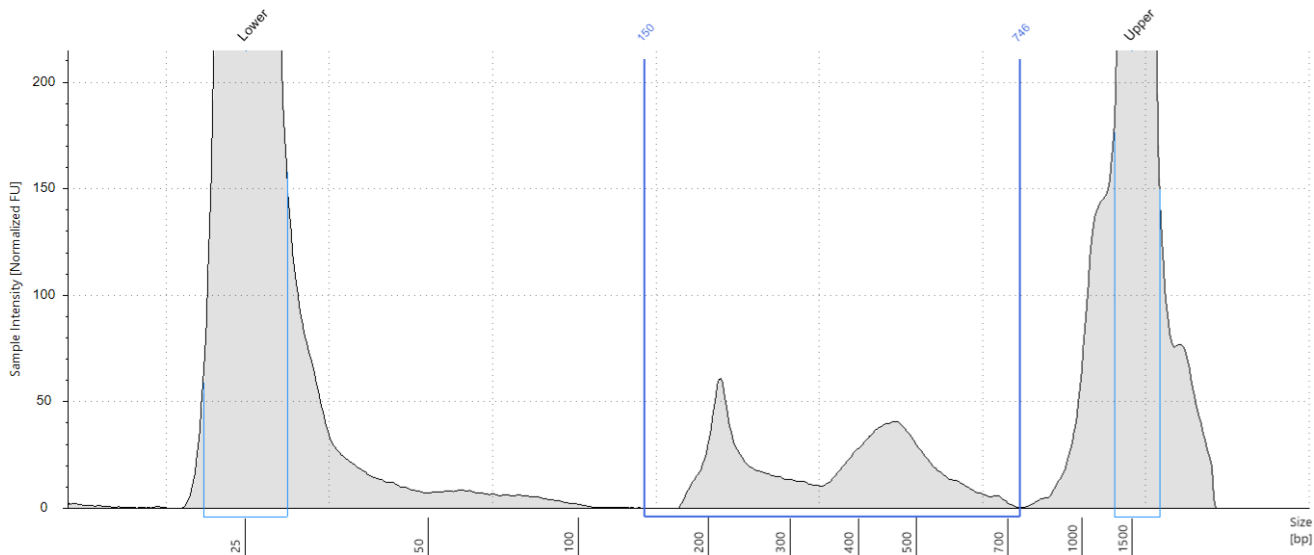

Region Table

From [bp]	To [bp]	Average Size [bp]	Conc. [ng/μl]	Region Molarity [nmol/l]	% of Total	Region Comment	Color
150	746	374	0.562	2.67	32.06		■